


Tue Feb 24 08:34:53 2004


TIDE Mass_0

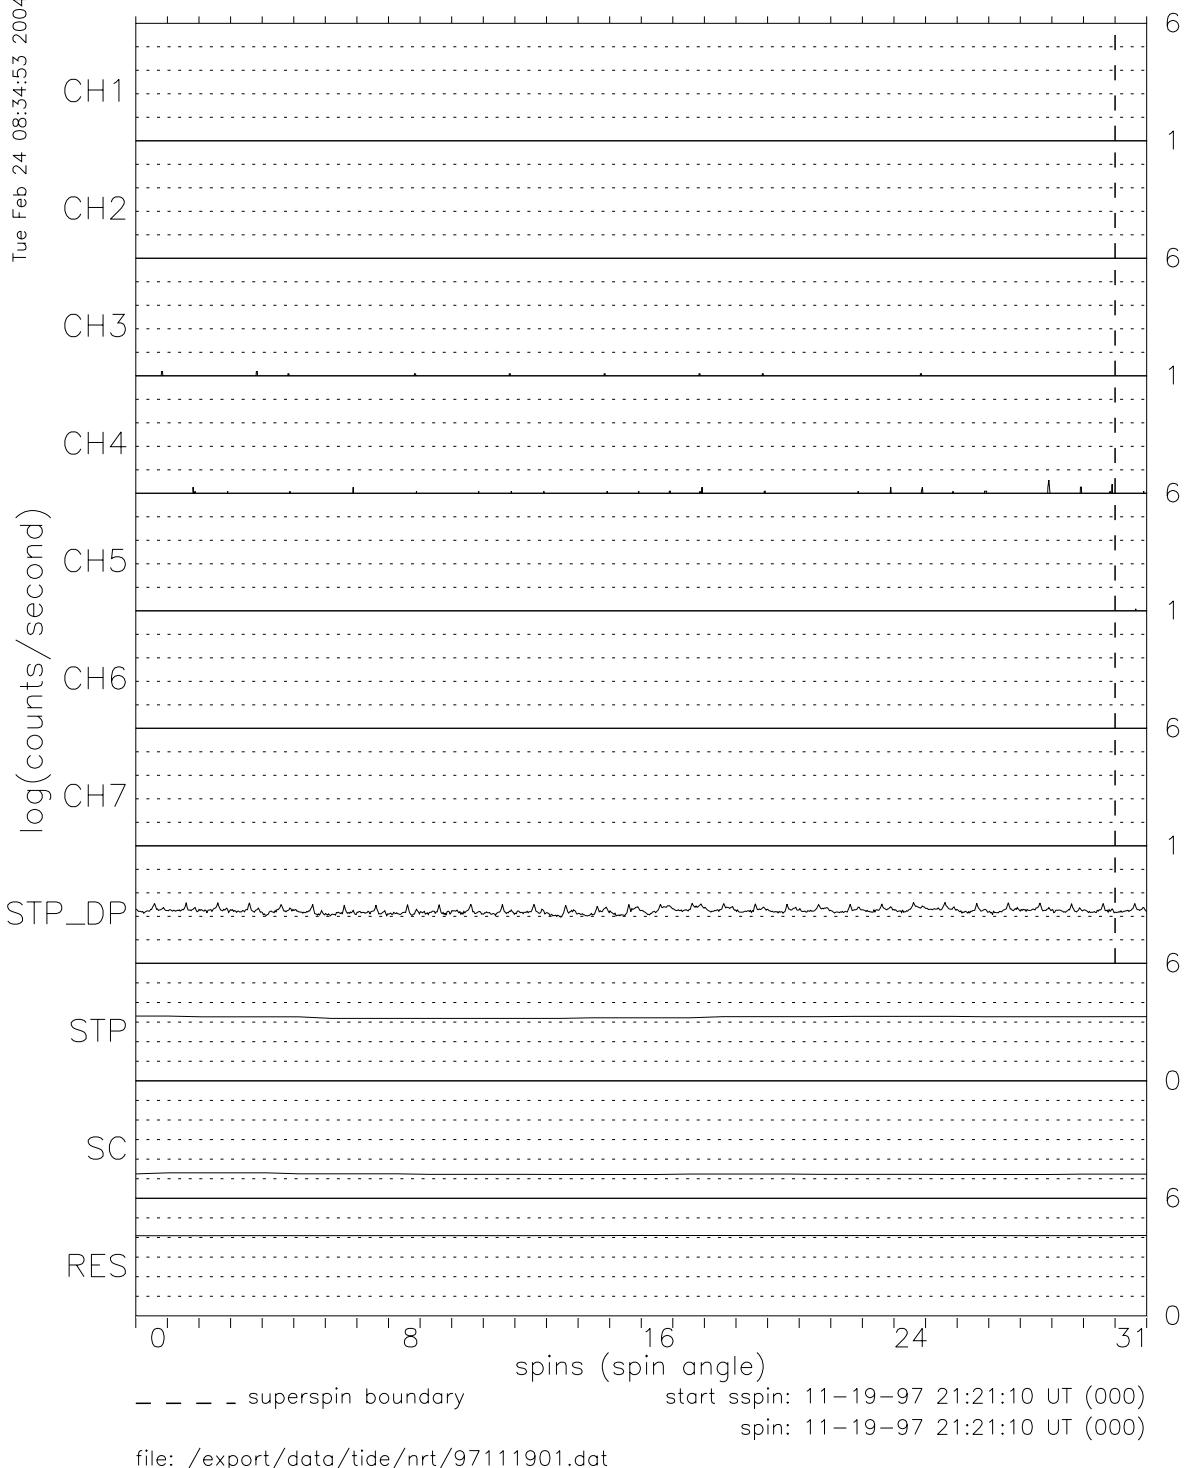

-15kV TOF: -9116 v
-3.6kV MCP: -2593 v
-2.4kV MCP: -1579 v
Input Cur: 302 ma
RPA max: 237 v
Mirror max: 238 v

Tue Feb 24 08:34:53 2004

TIDE Direct Events

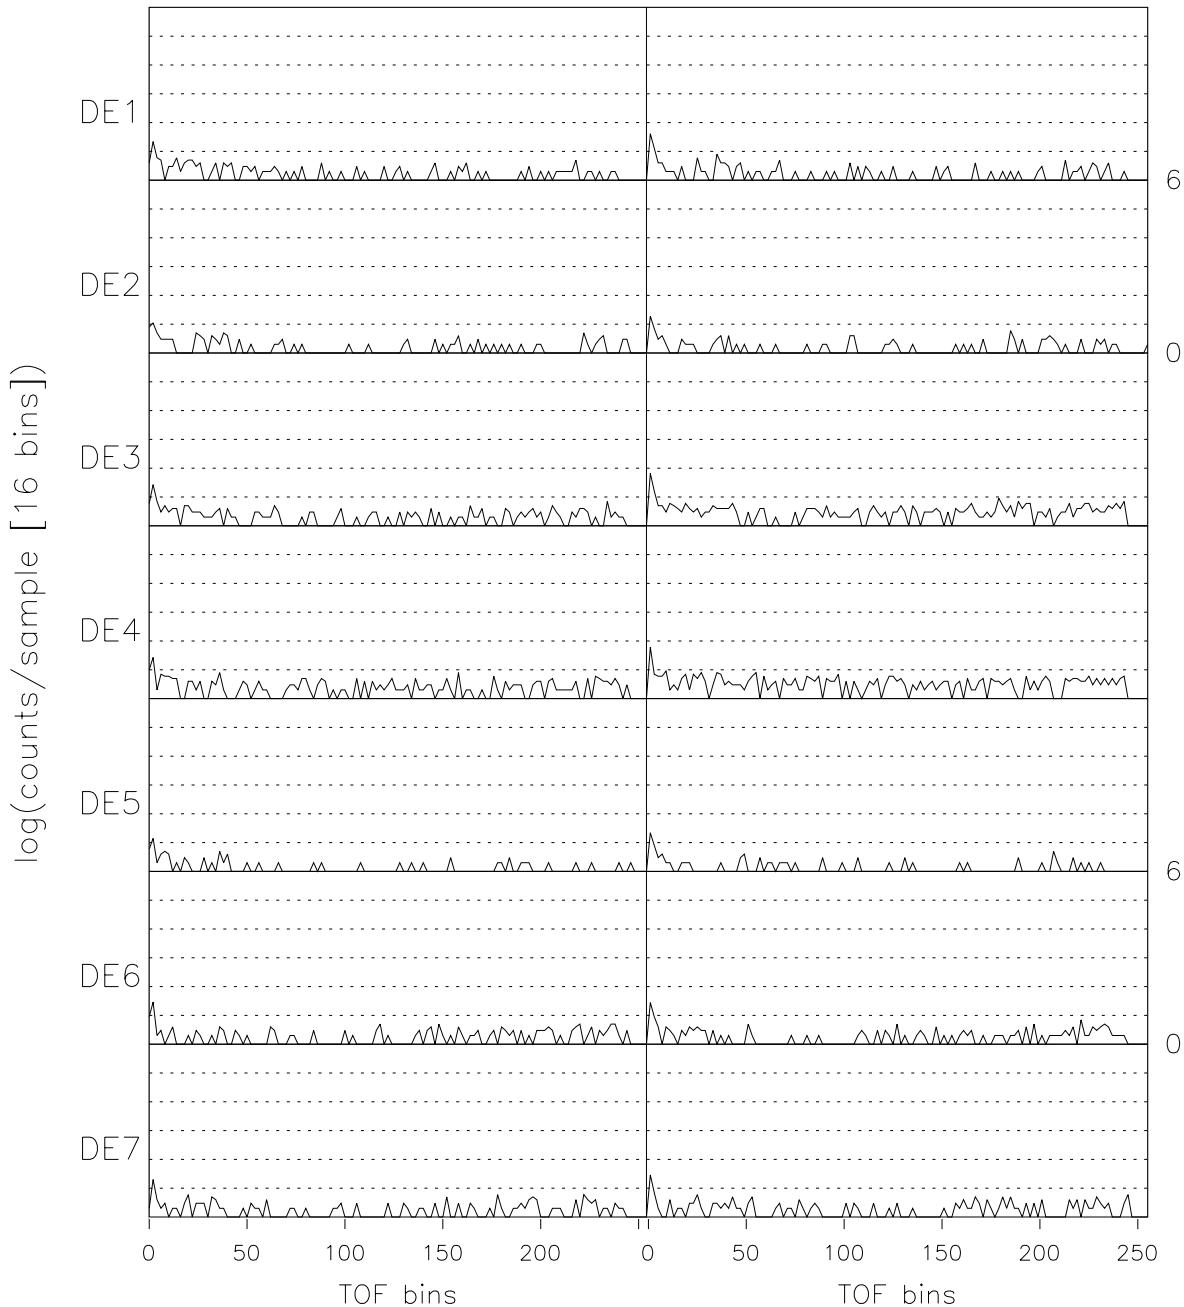

reported: 11-19-97 21:14:40 UT

reported: 11-19-97 21:17:52 UT

file: /export/data/tide/nrt/97111901.dat

-15kV TOF: -9245 v

-3.6kV MCP: -2578 v

-2.4kV MCP: -1579 v

Input Cur: 290 ma

RPA max: 237 v

Mirror max: 238 v